

BEST AVAILABLE COPY



Schematic view of analyzing service providing system

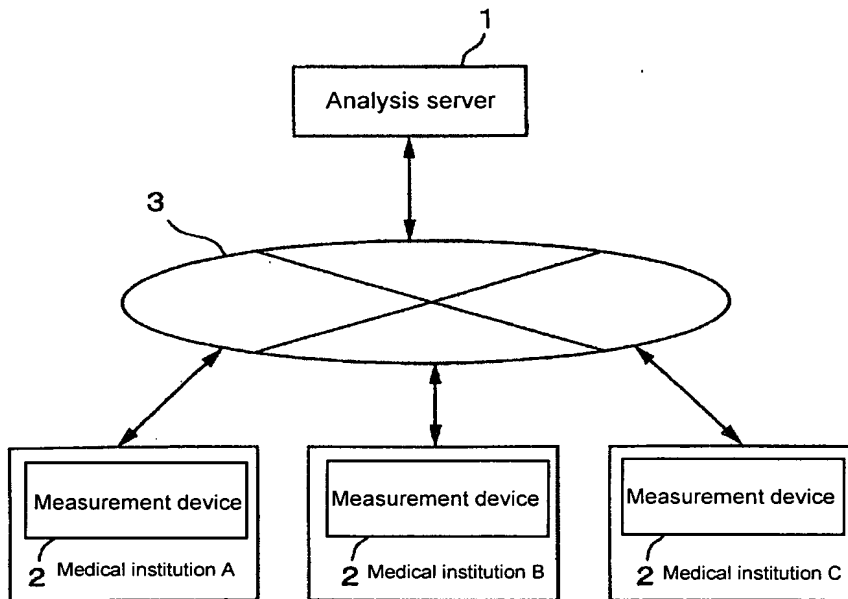


Fig. 1

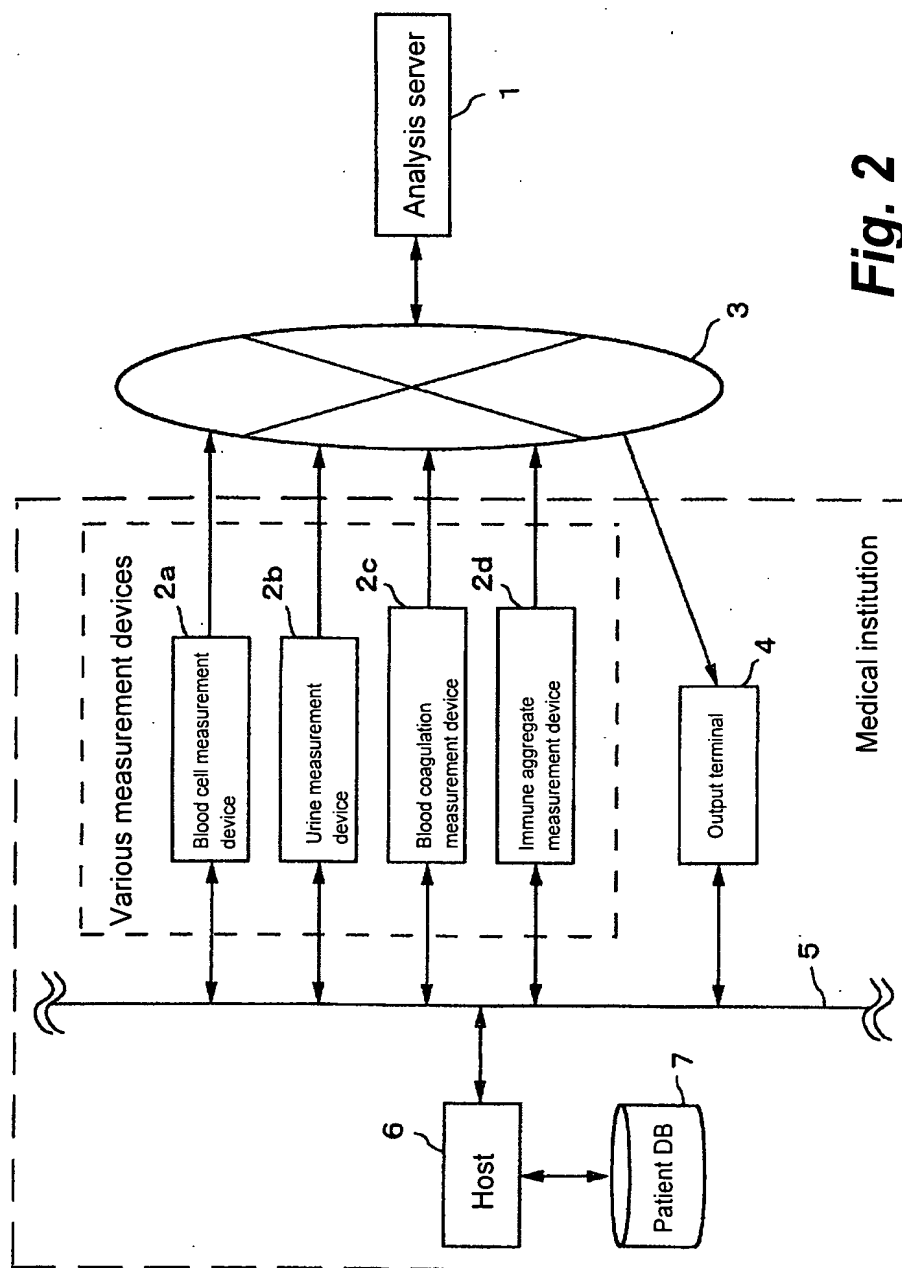


Fig. 2

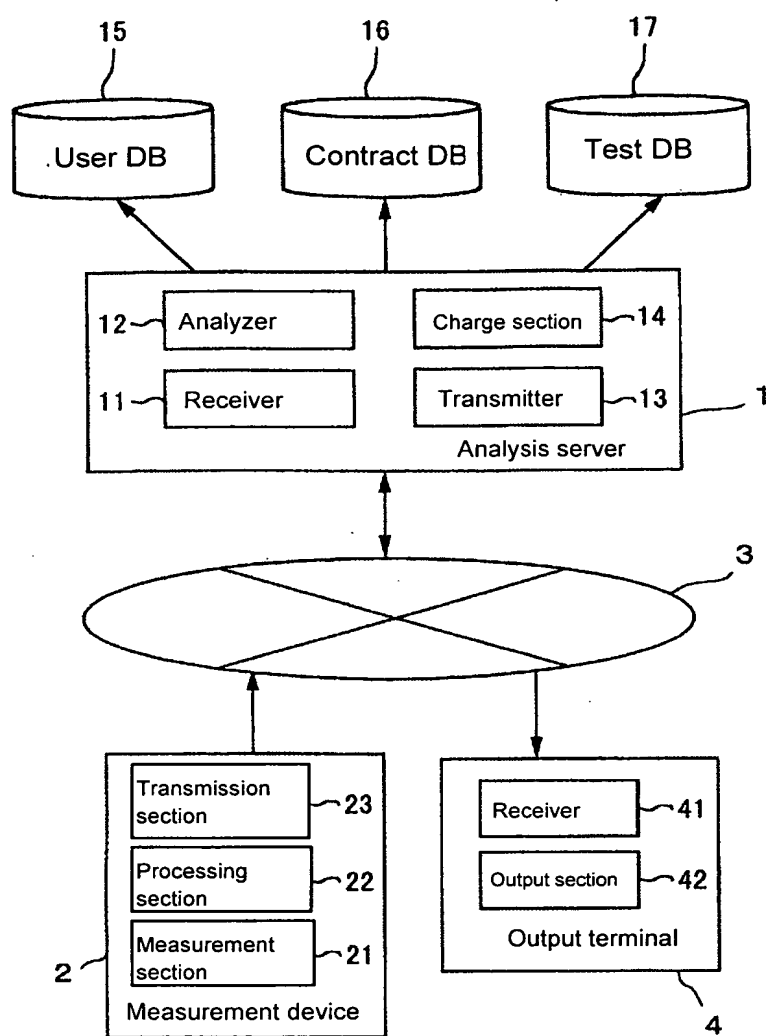


Fig. 3

Conceptual view of a user DB

User ID	U—sysmex
User Name	Sysmex Hospital
Contact Person	Test Dept.: Tanaka
Contract details	123-4567
Service usage	
BASIC	100
C001	60
C002	37

Fig. 4

Conceptual view of contact DB

Contract details	Analysis service	Test Items	Basic contract flag	Basic fee	Maximum
123-4567	C001	APTT, PT, Fbg	Yes	¥15,000	100
123-4567	C001	APTT, PT, Fbg	Yes	¥200	
123-4567	C002	TTO	No	¥450	

Fig. 5

User ID	U—sysmex
Specimen ID	01-001
Device ID	M103
Parsing order	6789
Sample classification	Blood
Test item	PT
Measurement item	PT
Device type	Sysmex CA-1500
Device version	Ver. 03
Reply address	out@U—sysmex. co. jp
Correction value	1
Measurement data	(2 sec. 28), (2.1 sec. 31), (2.2 sec. 35)

Fig. 6

Working data transmitted to output terminal from analysis server

User ID	U—sysmex
Specimen ID	01-001
Device ID	M103
Parsing order	6789
Sample classification	Blood
Test item	PT
Device version	Sysmex CA-1500
Analytical data	11.0 sec.
Supplemental Information	110.5% 1.04 1.07INR

Fig. 7

Flow of analysis process

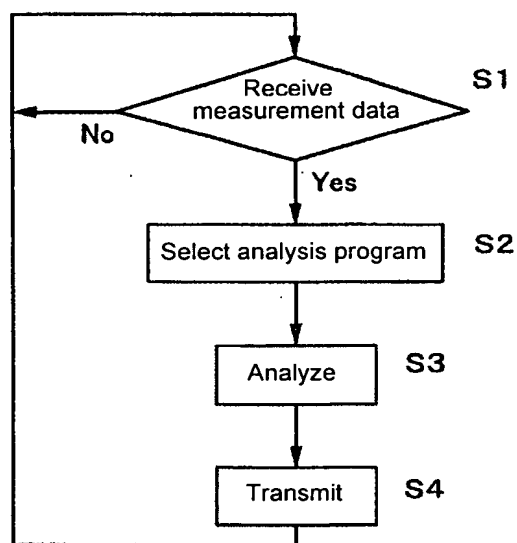


Fig. 8

Flow of charge process

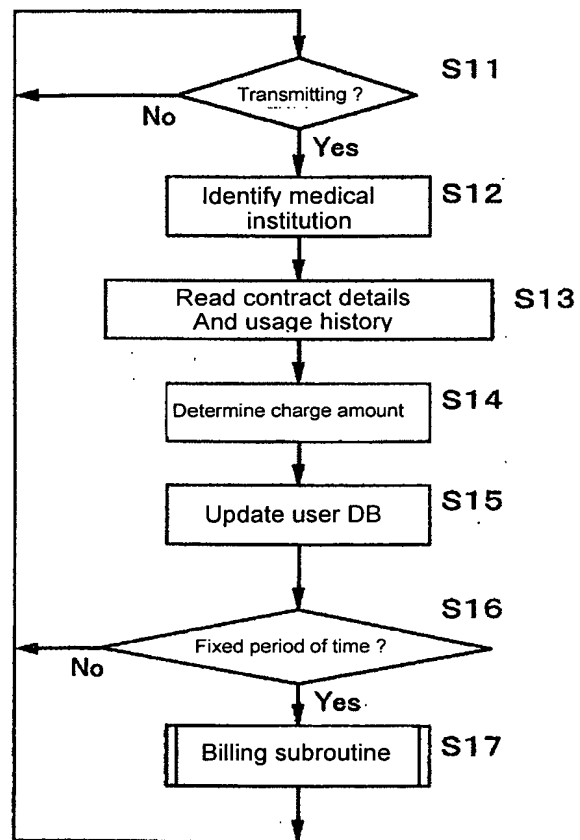


Fig. 9

Flow of billing process

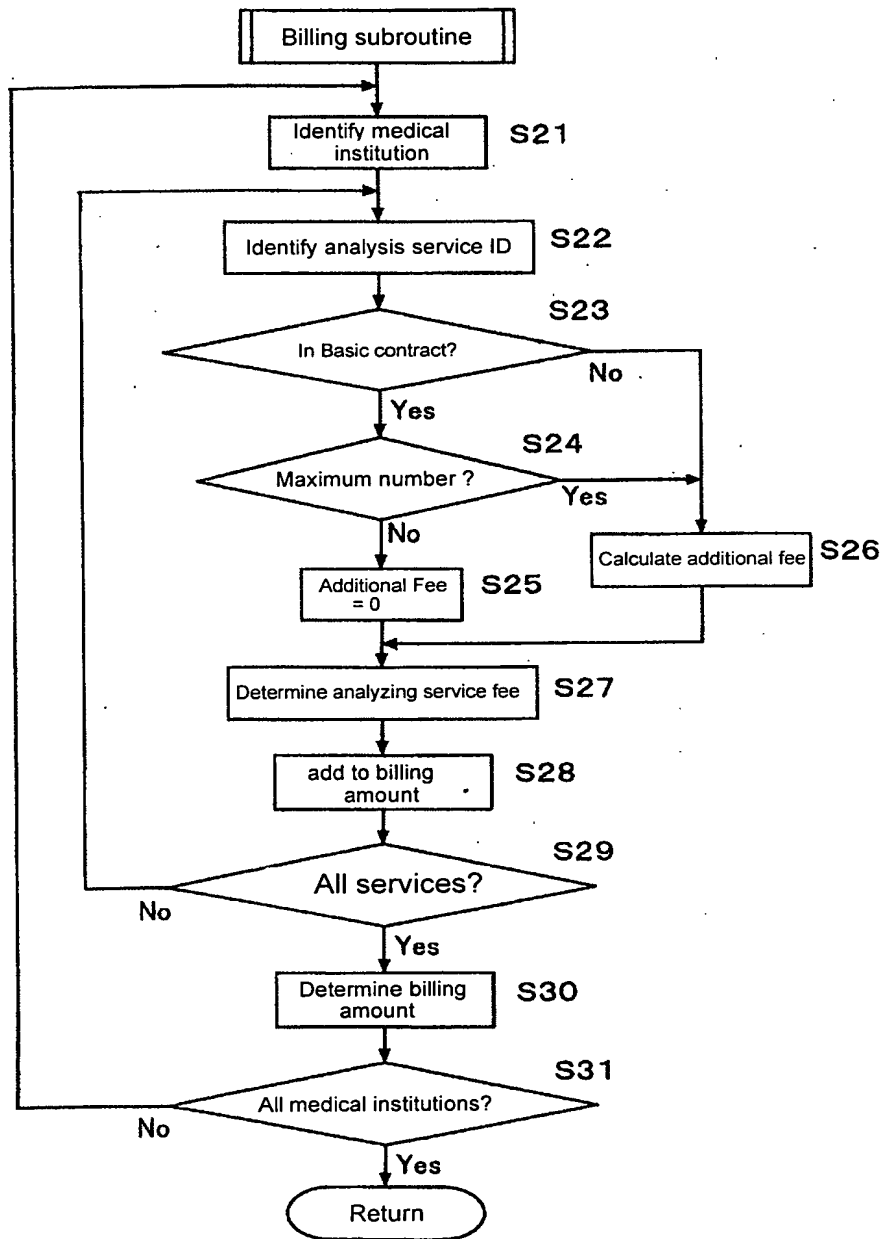


Fig. 10


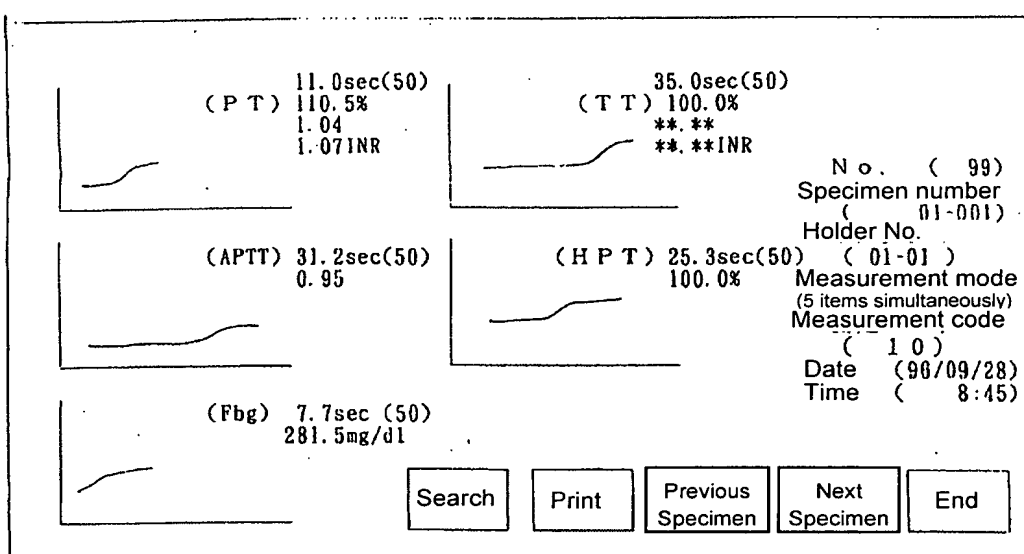


Fig. 11

Fig. 12

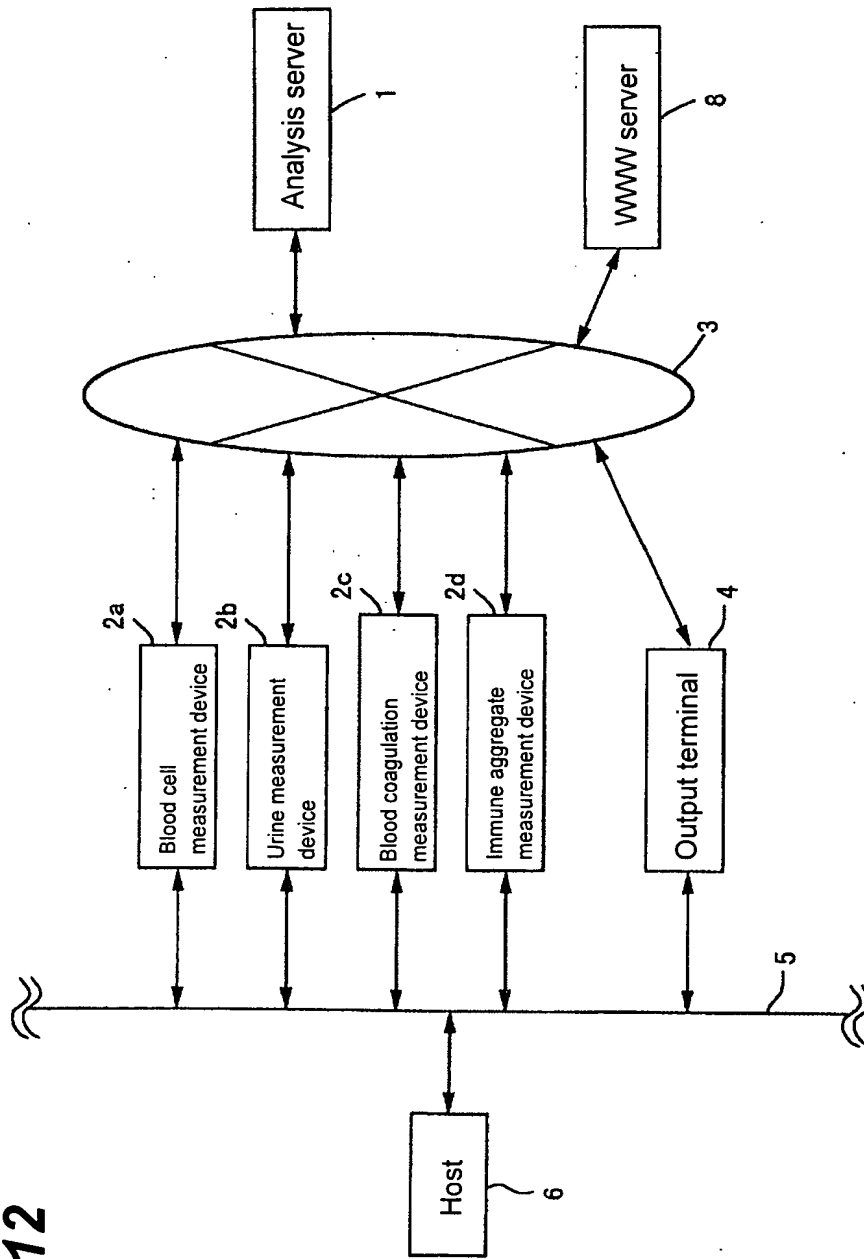

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☒ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.